


1/2

Fig. 1

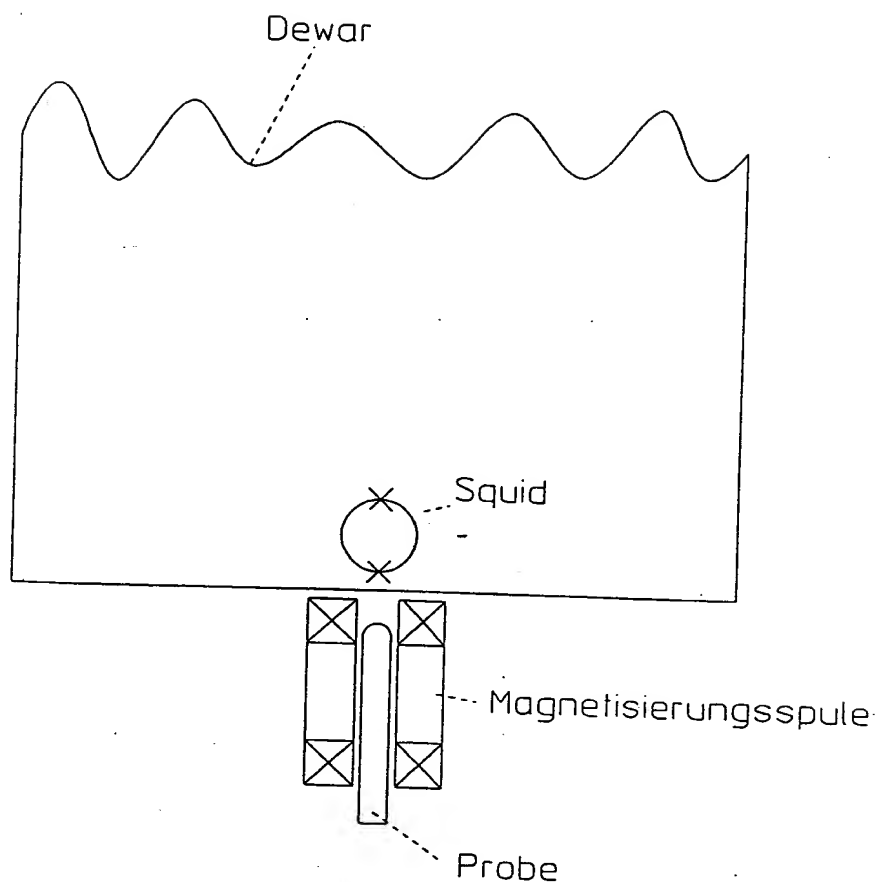

[Key:]

Dewar = Dewar

Squid = Superconducting Quantum Interference Device


Magnetisierungsspule = magnetizing coil

Probe = sample

Probe wird während der Messung entfernt = The sample is removed
during measurement

08/80473

Fig. 2

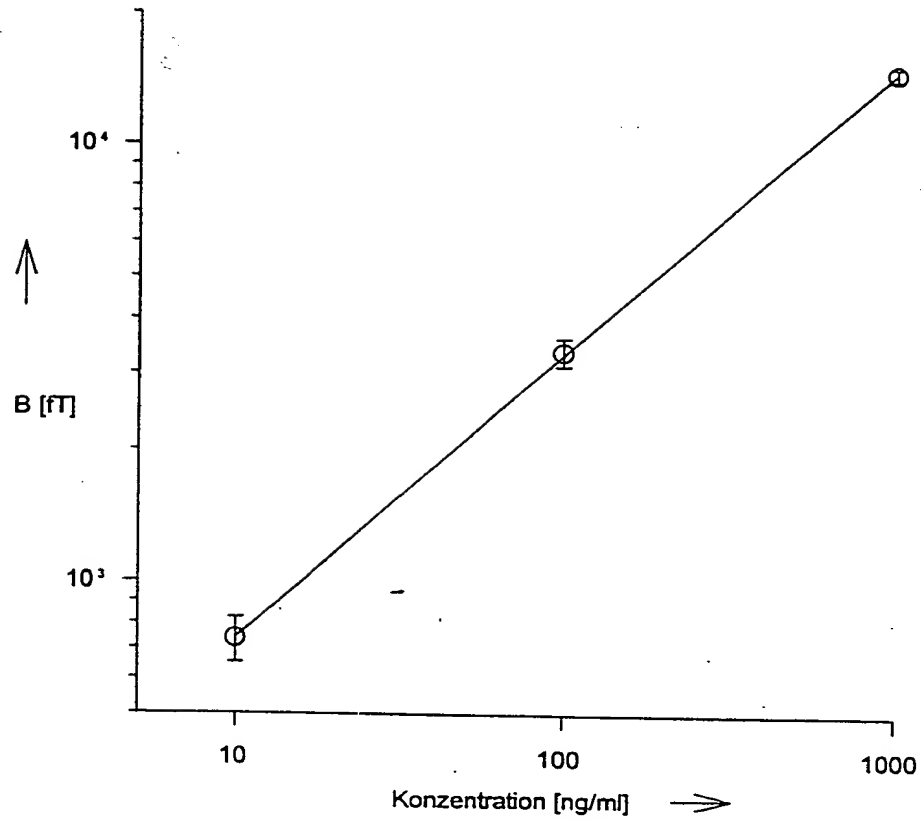

[Key:]

Konzentration [ng/ml] = concentration [ng/ml]